

# Instruction Manual

Upper Arm Electronic  
Blood Pressure Monitor  
Model No.: FC-BP121



Manual Ver.: 1.0

Issuing Date: 2022/08/02

- Please read this instruction manual carefully before using your unit.
- Please keep this instruction manual well for future use.
- Thanks for choosing the Digital Blood Pressure Monitor.
- The PATIENT is the designated OPERATOR.

# Contents

|   |           |
|---|-----------|
| Contents.....                           | 2         |
| <b>1. Before Using the Unit.....</b>    | <b>2</b>  |
| 1.1 Introduction.....                   | 2         |
| 1.2 Important safety notices.....       | 3         |
| 1.3 Warning and safety notices.....     | 4         |
| <b>2. Operating Instruction.....</b>    | <b>6</b>  |
| 2.1 Introduction of machine.....        | 6         |
| 2.2 Battery Installation / Removal..... | 7         |
| 2.3 Settings.....                       | 8         |
| 2.4 Proper Use of the Arm Cuff.....     | 9         |
| 2.5 Considerations for measurement..... | 11        |
| 2.6 Function.....                       | 12        |
| 2.7 Take a Measurement.....             | 12        |
| 2.8 Use the Memory function.....        | 13        |
| 2.9 About Blood Pressure.....           | 15        |
| <b>3. Care and Maintenance.....</b>     | <b>17</b> |
| 3.1 Care and Maintenance.....           | 18        |
| 3.2 Calibration and Service.....        | 18        |
| 3.3 Error Indicators.....               | 18        |
| 3.4 Troubleshooting.....                | 18        |
| 3.5 Technical Data.....                 | 19        |
| 3.6 Technical description.....          | 21        |
| <b>4. Warranty Information.....</b>     | <b>25</b> |

# 1. Before Using the Unit

## 1.1 Introduction

- Thank you for purchasing Upper Arm Electronic Blood Pressure Monitor.
- The unit uses the oscillometric method of blood pressure measurement. It means the unit detects the movement of your blood through your brachial artery, and converts your blood pressure into a digital reading. The unit is simple to use because a stethoscope is not needed while using an oscillometric monitor.
- The unit stores automatically 2\*120 sets of measurement values. You can read the stored data conveniently by pressing the memory button.
- The unit comes with the following components:
  - Main Unit
  - Arm Cuff
  - Instruction Manual printed in English

| SYMBOLS USED IN THIS INSTRUCTION MANUAL   |  |
|---|--|
|    | Indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.  |
|    | Indicates a potentially hazardous situation which, if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other property.             |
|   | Please read this instruction manual thoroughly before using the unit.<br>Please keep for future reference.<br>For specific information about your own blood pressure, CONSULT YOUR DOCTOR. |
|  | Transport package should be kept away from rain.   |
|  | AUTHORISED REPRESENTATIVE IN THE EUROPEAN COMMUNITY  |
|  | Refer to instruction manual/booklet  |
|  | MANUFACTURER   |

|   |   |
|---|---|
|    | SERIAL NUMBER   |
|   | Type BF applied part  |
|  | The marking of electrical and electronics devices according to Directive 2002/96/EC.<br>The device accessories and the packaging should be disposed of as waste correctly at the end of its service life<br>Please follow Local Laws or Regulations for disposal. |
|  | Device used in the Magnetic Resonance (MR) environment is prohibited.   |
|  | Manufacturing date  |
|  | Medical device  |

## 1.2 Important safety notices

To assure the correct use of the product basic safety measures, precaution should be followed as below:

- Please read all information in the instruction manual and any other literature included in the box before using the unit.
- Please contact your physician for specific information about your blood pressure.  
Self-diagnosis and treatment by measure results may be dangerous.  
Follow the instructions of your health care provider.
- Operate the unit only as intended. Don't use for any other purpose.  
The unit is intended to use for measuring blood pressure and pulse rate for adult only, not recommended using for neonatal baby at home or medical centre.
- Do not use a cellular phone near the unit. It may result in operational failure.
- Please avoid using in high radiant area in order to have a correct reading.

- Do not disassemble or attempt to repair the unit or components. Do not use the equipment in places where there are flammable gas (such as anesthetic gas, oxygen or hydrogen) or flammable liquid (such as alcohol) .
- Do not use a mobile phone or other devices that emit electromagnetic fields near the unit. This may result in incorrect operation of the unit.
- There will be indication that too frequent measurements can cause injury to the PATIENT due to blood flow interference;
- Please do not put CUFF over a wound, as this can cause further injury;
- Please pay attention to the effect of blood flow interference and resulting harmful injury to the PATIENT caused by continuous CUFF pressure due to connection tubing tangling;
- Statement: Regarding the requirements of the adapter, it should meet the following conditions, output voltage: DC 5V, Current: 1000mA, and comply with IEC 60601-1 and IEC 60601-1-11, provide two MOPP insulation between ac input and dc output.
- Please install the battery properly.
- When the battery power is off, please replace four new batteries.
- If over three months do not use the device, please remove the battery as it may cause leakage, overheat, rupture and damage the blood pressure monitor casing.



### **1.3 Warning and safety notices**

- Regarding the application of the CUFF and its pressurization on any limb where vascular access or therapy, or an arteriole-venous (A-V) shunt, is present because of temporary interference to blood flow and could result in injury to the PATIENT;


- Regarding to the application of the CUFF and its pressurization on the arm on the side of a Brachial Artery;
- Pressurization of the CUFF can temporarily cause loss of function simultaneously used monitoring ME EQUIPMENT on the same limb;
- Regarding the need to check (for example, by observation of the limb concerned) that operation of the AUTOMATED Blood Pressure Monitor does not result in prolonged impairment of the circulation of the blood of the PATIENT.
- When the arm is oppressed by air pressure, please loosen CUFF or remove batteries.
- Please do not touch the patient and battery output simultaneously when measuring.
- Warning: Do not allow to use the lure connectors. If lure lock connectors be used in the construction of tubing, there is a risk that they might be inadvertently connected to vascular fluid systems and allowing air to be pumped into a blood vessel.
- Warning: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Blood Pressure Monitor, including cables specified by the manufacturer. Otherwise, weakening of the performance of this equipment could cause.
- Warning: Keep BPM out of reach of children and animals.
- Warning: A child or animal is strangled due to the too long air hose.
- Warning: The risk of accidental ingestion due to the small parts that can be disassembled (such as batteries, etc.) after being touched by a child;  
Place the product out of the reach of children, etc.; use it under the supervision of an adult, etc.

## 2. Operating Instruction

### 2.1 Introduction of machine Body

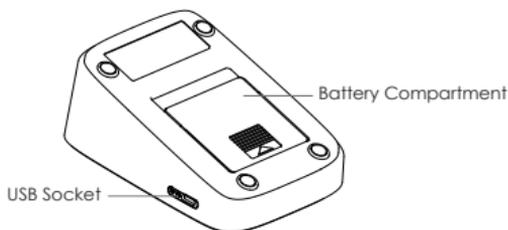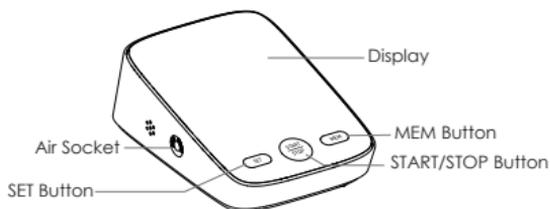


### Display

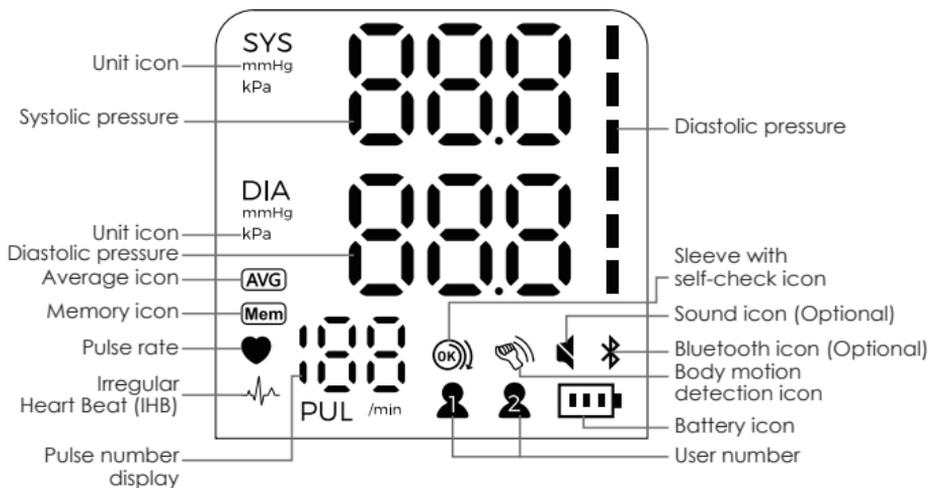

## Arm Cuff


- Fit for 9-17 inches (22cm~42cm) range of upper arm perimeter

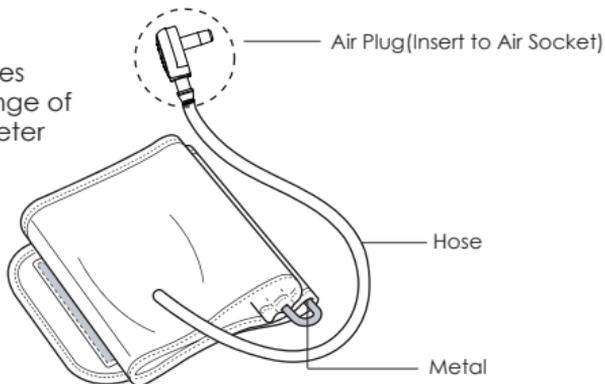

- ⚠ If your arm cuff is broken or not functional, please use a new cuff.
- ⚠ A new arm cuff does not include an air plug. Please continue to use the old air plug on the new arm cuff.

## Power

4 AAA Alkaline Batteries



- ⚠ Do not use rechargeable batteries.

## Instruction Manual

- Please keep the instruction manual well after using.


### 2.2 Battery Installation / Removal

2.2.1 Remove the battery cover from the battery compartment.

2.2.2 Install 4 "AAA" size batteries to match the + (positive) and -

(negative) polarities with the polarities of the battery compartment as indicated.

2.2.3 Replace the battery cover.

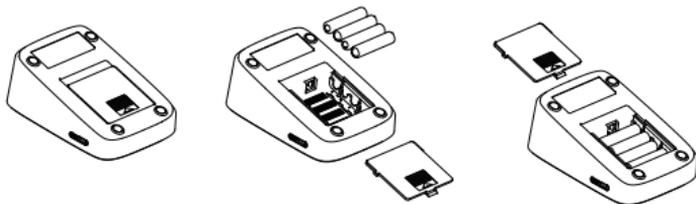

### ⚠ Caution!


- Replace batteries if the symbol of low battery power appears on the display.
- Never leave any low power battery in the battery compartment since they may leak and cause damage to the unit.

## 2.3 Settings

### 2.3.1 To set voice

Long press the " SET " button when power off, you can see the " " icon appears and flashes, then press the " MEM " button to adjust the sound on or off. When the screen shows "  $\overset{SP}{ON}$  ", Blood Pressure Monitor sound is on; when the screen shows "  $\overset{SP}{OFF}$  ", Blood Pressure Monitor sound is off.

Press " START/STOP " button to save the current setting and turn off.

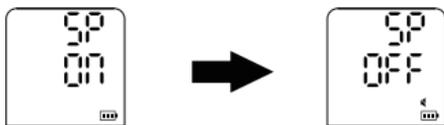

### 2.3.2 To set unit


Based on the first step and press the "SET" button to change the previous unit(kPa or mmHg), the mark "  $\frac{0}{0}$  " appears and flashes, now the BPM is in mmHg status, and then press the " MEM " button, to change it into "  $\frac{00}{00}$  ", now the BPM is in kPa status.

Press the " START/STOP " button to confirm the current setting.




### 2.3.3 To set user

Press the " SET " button when powered off, and then press the " SET " button again to switch User 1 or User 2.

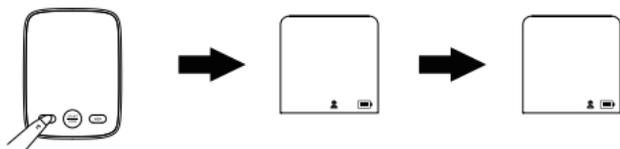

### 2.4 Proper Use of the Arm Cuff

2.4.1 Make sure the air plug is inserted properly in the main unit.

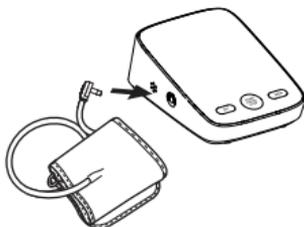

2.4.2 Remove all clothes from your upper arm allowing the cuff to fit directly on the skin.



2.4.3 Sit in a chair with your feet flat on the floor. Place your arm on a table so as to level the cuff to your heart.




2.4.4 Pass the hose through the metal, and keep the hose outward.



2.4.5 Put your arm through the loop, then pull it up to the position of your upper arm.




2.4.6 The hose runs down the inside of your arm. The bottom of the cuff should be approximately 0.8-1.2 inches (2~3cm) above your elbow.

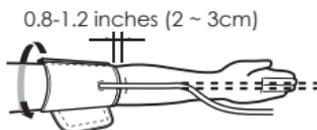

2.4.7. Wrap the cuff tightly around your upper arm by using the arm band. Make sure at least there should be 1-2 fingers space between arm and cuff.

Any piece of clothing restricts the arm which must be taken off.



2.4.8 Relax your arm, keep the palm upward and the fingers curving naturally, then turn on the unit and start to measure.



## 2.5 Considerations for measurement

### 2.5.1 The correct using method


(1) Elbow on the table; comfortably seated; legs uncrossed; back and arm supported;

(2) Keep the center of the cuff and the heart or nipples at the same height.

(3) Do not put the clothes into the cuff.

(4) Palms up, and keep relaxed.

(5) Sitting in a chair keep your foot flat on the ground.

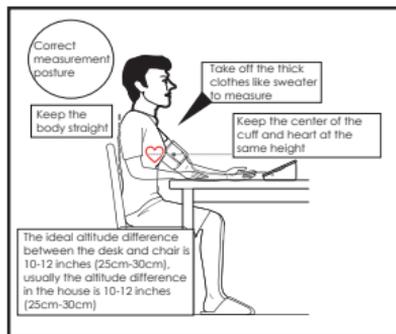

A recommendation that the PATIENT should be relaxed and not talk during the measurement PROCEDURE; a recommendation that 5 min elapses before the first reading is taken; need to avoid compression or restriction of the connection tubing.

### 2.5.2 Ideal environment for measuring blood pressure

(1) Get up in the morning, and the mood is relaxed.

(2) No consciousness to the toilet.

(3) Room temperature is about 20 °C.

(4) A quiet place where there was no noise around.

2.5.3 Measure blood pressure at the same time every day: Blood pressure is constantly changing and cannot judge the situation only by the result of once blood pressure measurement for a period of time, repeated measurements to determine blood pressure condition is more reliable So please stick to measuring blood pressure every day, select the mood in a day can keep the most stable state such as early in the morning after getting up.

Ideal method is to measure as far as possible at the same time every day.

Note: Be sure to have more than 2-3-minutes interval between two measurements.


Depending on your individual physiological characteristics, between the two measurements may need to rest for a longer time. Please keep the cuff around your arm before you start measuring. Do not measure your blood pressure on the bus.

## 2.6 Function

- 2.6.1. The device has the WHO warning strip "■" symbol display function, with the blood pressure value change, the higher blood pressure value "■" symbol will appear relatively in the higher position (refer to WHO definition of high blood pressure levels-reference table).
- 2.6.2. The device has the average of the last three display function (press the memory key for the first time to display the value that is the average of the last three measurements).
- 2.6.3. The device has a large screen display and legible digital reading.
- 2.6.4. The device has kPa and mmHg display switching and measurement functions.
- 2.6.5. The device has double memory lookup function and can store 120 sets of measurements for each person to remember the normal status of your blood pressure.
- 2.6.6. Low power detection: detecting low power under any working circumstance, LED displays "☐" symbol indicates low power.
- 2.6.7. Overpressure protection function: when the pressure is more than 300mmHg, the device cause automatic power consumption fastly.
- 2.6.8. Automatic shutdown function: The device will shut down automatically if it is without operation for 2 minute.
- 2.6.9. Heartbeat prompting function.
- 2.6.10. Prompting voice of completed measurement.
- 2.6.11. Incorrect prompting function.

## 2.7 Take a Measurement

- 2.7.1 Press the " START/STOP " button.  
All display symbols appear on the screen. The cuff starts to inflate automatically.

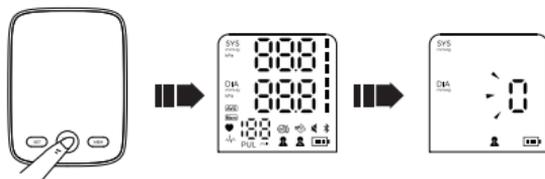

2.7.2 Measurement start. When pressurized to stop blood flow, the Blood Pressure Monitor stops pressure before automatically leaking air and measuring blood pressure.

The heartbeat symbol flashes when a pulse is detected.

When the heart beat symbol appears and flashes, the Blood Pressure Monitor detects the pulse and begins to calculate the pulse automatically.



2.7.3 The blood pressure and pulse rate are displayed when the measurement completed.

The cuff is deflated automatically, and all of the measurement results are stored in the memory.

The "⚡" symbol will be displayed if irregular heartbeat is detected.



2.7.4 Press the "START/STOP" button to turn off the unit.

The unit will be automatically turned off after two minutes if no more operation.

NOTE: The inflation or measurement can be stopped by pressing the "START/STOP" button at any time.


## 2.8 Use the Memory function

The unit stores the blood pressure and pulse rate in the memory mode after completing a measurement each time. 2x120 sets of measurement values can be stored automatically.

The earliest record will be deleted automatically to save the latest measurement value when more than 2x120 sets.

The unit also calculates an average reading based on the values of the latest 3 times measurement .


2.8.1 To enter the memory mode & to read the average value  
Press the " MEM " button while the unit is off, the unit it becomes the memory mode and the average value of the latest 3 times measurement values of the current user will be displayed.

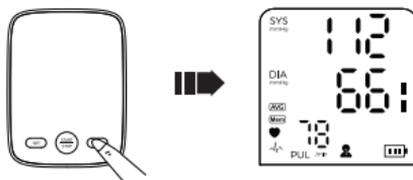

2.8.2 To read the measurement value

Press the " MEM " button when powered off, the latest measurement values will be displayed.


Press the " MEM " button once more, the measurement values before the latest will be displayed, and so on.

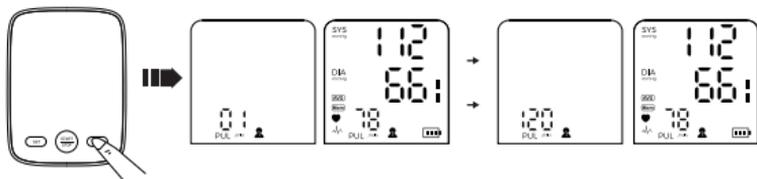

2.8.3 To delete the memory value

■ In the memory mode, long press the " MEM " button, the unit displays the following symbol to cancel all the memory records of the current user.

■ Please operate the delete memory function cautiously.

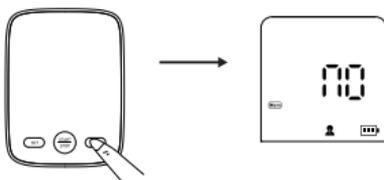


## 2.9 About Blood Pressure

### 2.9.1 Irregular Heartbeat Symbol IHB

When the unit detects an irregular rhythm two or more times during the measurement, the irregular heartbeat Symbol will appear on the display with the measurement values.

An irregular heartbeat rhythm is defined as a rhythm that is more than 25% slower or 25% faster from the average rhythm which detected while the monitor is measuring the systolic blood pressure and the diastolic blood pressure.

If the Irregular Heartbeat Symbol (  ) displays your measurement results, we recommend you consult your physician, and follow the doctor's directions.

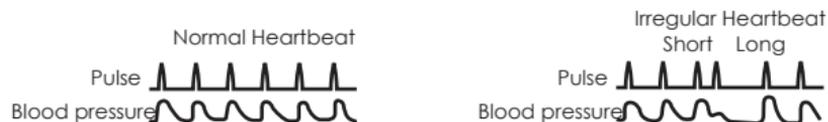


### 2.9.2 Blood Circulation

The blood circulation is responsible for supplying the body with oxygen.

Blood pressure is the pressure exerted on the arteries.


The systolic blood pressure value (higher pressure or top value) represents the blood pressure produced by contraction of the heart muscle.

The diastolic blood pressure value (lower pressure or lower value) represents the blood pressure produced by relaxation of the heart muscle.

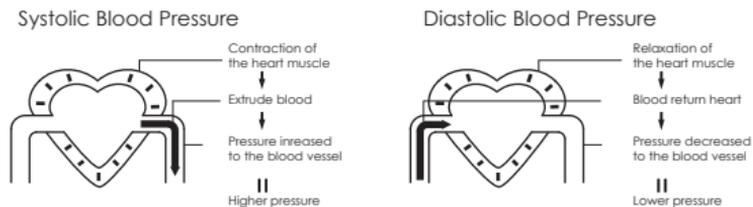

### 2.9.3 Health and Blood Pressure


The incidence of hypertension increases with age. In addition, if a lack of exercise, excess body fat and high levels of cholesterol(LDL), would sticks to the inside of blood vessels, which reduces elasticity of these vessels. Hypertension accelerated arteriosclerosis which can lead to serious conditions such as stroke and myocardial infarction. For these reasons, it is very important to know whether the blood pressure is within a healthy range. Blood pressure fluctuates from minute to minute throughout the day. Therefore it is essential to take regular measurements to help you identify an average blood pressure.

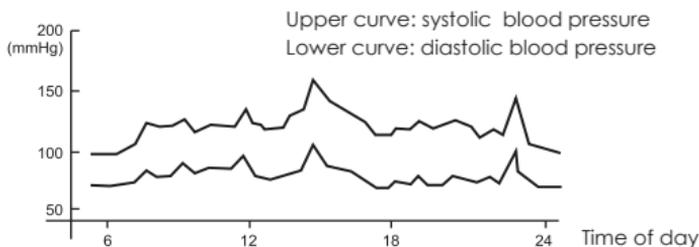

### 2.9.4 Classification of Blood Pressure

After each measurement is completed, the LED display will show your position automatically on the six segments of the bar indicator which corresponds to World Health Organization (WHO) Blood Pressure Indicator.

Reference Material: Journal of Hypertension 1999, Vol 17 No.2

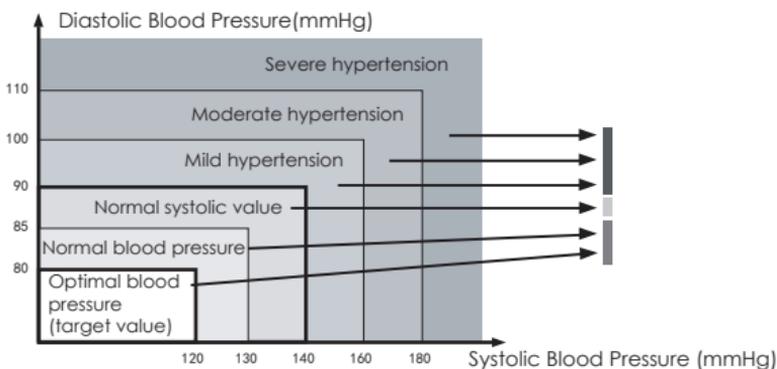

**\*Note!**

When a person's systolic and diastolic pressures fall into different categories, the higher category should apply.

### 2.9.5 Symptoms of High Blood Pressure

High blood pressure can go unnoticed for a long time, since it doesn't cause noticeable symptoms. The following are possible causes of abnormally high blood pressure:

- Overweight;
- High cholesterol level;
- Smoking;
- Excessive alcohol consumption;
- Stress and emotional upset;
- Excessive consumption of salt;
- Lack of physical exercise;
- Genetic / hereditary predisposition;
- Underlying illnesses, such as kidney disorders or endocrine disturbance.

### 2.9.6 Treatment of High Blood Pressure

If your blood pressure reaches upper values of 140~160 mmHg and lower values of 90~95 mmHg in repeated measurements over several days, you should consult doctor for detailed medical examination. You can assist the treatment prescribed by your doctor in the following ways:

- Lose weight and lower your cholesterol level;
- Reduce the consumption of alcohol;
- Reduce the intake of salt;
- Stop smoking;
- Take regular exercise;
- Monitor your blood pressure.

## 3. Care and Maintenance

### 3.1 Cleaning/Disinfecting and Maintenance

To keep your blood pressure monitor in the best condition and protect the unit from being damaged, please follow the directions listed below:

3.1.1 Clean the blood pressure monitor frequently after used by a user.

Do not use any abrasive or volatile cleaners. Never immerse the unit or any components in water.

3.1.2 Use a soft dry cloth towel to clean this blood pressure monitor if it is very filthy you can wet the towel with water or neutral detergent, wring out it and wipe the monitor.

3.1.3 Disinfection the cuff with moistened 95% alcohol cotton wool.

3.1.4 Store the unit in a safe and dry location. Do not fold the cuff too tight. Do not expose the unit to extreme hot or cold temperatures/humidity and do not expose the unit under the direct sunlight.

3.1.5 Avoid subjecting the unit to strong shocks, such as dropping the unit on the floor.

3.1.6 Remove the batteries if the unit will not be used for three months or longer. Always replace all the batteries with new ones at the same time.

3.1.7 Use the unit based on the instruction provided in this manual.

Only use authorized parts and accessories.

3.1.8 Do not repair or open the machine by yourself. If a defect occurs, Please contact the local distributor.

3.1.9 We will provide circuit diagrams, component part lists, descriptions, calibration instructions, or other information to assist service personnel who is trained by the manufacturer and has got the relevant qualification certificate.

### 3.2 Calibration and Service

The accuracy of this blood pressure monitor has been carefully tested and is designed for a long service life. It is generally suggested to have the unit inspected every two years to ensure correct functioning and accuracy. Please consult local authorized distributor or dealer.

### 3.3 Error Indicators

The following symbols will appear on the display when measuring abnormally.

| Symbol  | Cause                                 | Correction  |
|---|---------------------------------------|---|
|   | The course of inflating appears error | Wrap the cuff correctly and tightly<br>Inflate over again after ensuring                    |
|   | When measurement fails                | Do not move your arm and body and keep quiet<br>Measure over again according to correct way |
|  | When the batteries power is too low   | Replace all of the worn batteries with new ones   |

### 3.4 Troubleshooting

| Problem  | Causes and Solutions  |
|--|---|
| No power   | Replace all of the exhausted batteries with new ones  |
| No digital reading appears on the display screen | Check that whether the battery is installed on the right polarity.  |
| Measurement values appear too high or too low    | Blood pressure varies constantly. Many factors may effect your blood pressure, including stress, time of day, how you wrap the cuff. Review the sections "Proper Way of Measurement" and "Take a Measurement" |

### 3.5 Technical Data

#### 3.5.1 Specifications

|    |                               |   |
|----|-------------------------------|---|
| 1  | Model                         | FC-BP121  |
| 2  | Measurement Method            | Oscillometric measurement method  |
| 3  | Display                       | LED Digital Display   |
| 4  | Measurement Range             | Blood Pressure range: 0~299mmHg (0 kPa - 39.9 kPa)<br>Pulse: 40 to 180 beats/min  |
| 5  | Accuracy of the cuff pressure | Static Pressure: $\pm 3$ mmHg( $\pm 0.4$ kPa)<br>Pulse rate: Within $\pm 5\%$ of reading  |
| 6  | Inflation                     | Automatic inflation by pump   |
| 7  | Deflation                     | Automatic rapid deflation   |
| 8  | Pressure Detection            | Semiconductor pressure sensor   |
| 9  | Memory                        | 2 Users * 120 memories  |
| 10 | Power supply                  | 4 AAA alkaline batteries ( not included ), DC6V<br>USB Type C (DC5V1A)  |
| 11 | Battery life                  | Approximately 300 measurements when using alkaline batteries at the room temperature of 22°C and by using three times a day and inflating to 170 mmHg |
| 12 | Storage Condition             | Temperature: -4°F to 140°F (-20°C to 55°C)<br>Humidity: 0 to 95% RH<br>Atmospheric pressure: 70 - 106kPa  |
| 13 | Operating Condition           | Temperature: 50°F to 104°F (10°C to 40°C)<br>Humidity: 15 to 85% RH   |
| 14 | Automatic Power-OFF           | Within 2 Minutes  |
| 15 | Weight of Main Unit           | 240g (exclude batteries)  |
| 16 | External Dimensions           | 129 X 96 X 53 mm  |
| 17 | Cuff                          | 9-17 inches (22-42cm)   |
| 18 | Electric Shock Protection     | Internal power supply appliance type B  |

|    |                        |                          |
|----|------------------------|--------------------------|
| 19 | Accessorial Components | Cuff, Instruction Manual |
| 20 | Service Life           | 5 Years                  |

To improve performance, these specifications are subject to change without notice.

The device, accessories and the packaging should be disposed of as waste correctly at the end of its service life, so that the risk of patient or user can be lowered to an acceptable level.

### **3.5.2 IEC 60601-1-2:2014/AMD1:2020 ME EQUIPMENT and ME SYSTEMS identification, marking and documents for Class B product**

Instructions for use

The ME EQUIPMENT or ME SYSTEM is suitable for home healthcare environments and so on.

**Warning:** Don't near active HF surgical equipment and the RF shielded room of an ME system for magnetic resonance imaging, where the intensity of EM disturbances is high.

**Warning:** Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

**Warning:** Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation."

**Warning:** Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Upper Arm Electronic Blood Pressure Monitor, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

**If any:** A list of all cables and maximum lengths of cables (if applicable), transducers and other ACCESSORIES that are replaceable by the RESPONSIBLE ORGANIZATION and that are likely to affect compliance of the ME EQUIPMENT or ME SYSTEM with the requirements of Clause 7 (EMISSIONS) and Clause 8 (IMMUNITY). ACCESSORIES may be specified either generically (e.g. shielded cable, load impedance) or specifically (e.g. by MANUFACTURER and EQUIPMENT OR TYPE REFERENCE).

**If any:** The performance of the ME EQUIPMENT or ME SYSTEM that was determined to be ESSENTIAL PERFORMANCE and a description of what the OPERATOR can expect if the ESSENTIAL PERFORMANCE is lost or degraded due to EM DISTURBANCES (the defined term "ESSENTIAL PERFORMANCE" need not be used).

### 3.6 Technical description

1.all necessary instructions for maintaining BASIC SAFETY and ESSENTIAL PERFORMANCE with regard to electromagnetic disturbances for the excepted service life.

2. Guidance and manufacturer's declaration -electromagnetic emissions and Immunity.

Table 1

| Guidance and manufacturer's declaration - electromagnetic emissions |            |
|---|------------|
| Emissions test  | Compliance |
| RF emissions CISPR 11   | Group 1    |
| RF emissions CISPR 11   | Class B    |
| Harmonic emissions IEC 61000-3-2                                    | Class A    |
| Voltage fluctuations/ flicker emissions IEC 61000-3-3               | Compliance |

Table 2

| Guidance and manufacturer's declaration - electromagnetic Immunity                                     |  |  |
|--|--|--|
| Immunity Test  | IEC 60601-1-2 Test level   | Compliance level   |
| Electrostatic discharge (ESD)<br>IEC 61000-4-2   | ±8 kV contact<br>±2 kV, ±4 kV, ±8 kV,<br>±15 kV air  | ±8 kV contact ±2 kV,<br>±4 kV, ±8 kV, ±15 kV air   |
| Electrical fast transient/burst<br>IEC 61000-4-4   | Power supply lines:<br>±2 kV 100 kHz<br>repetition frequency   | Power supply lines:<br>±2 kV 100 kHz<br>repetition frequency   |
| Surge IEC 61000-4-5  | line(s) to line(s): ±1 kV.   | line(s) to line(s): ±1 kV.   |
| Voltage dips, short interruptions and voltage variations on power supply input lines<br>IEC 61000-4-11 | 0% 0.5 cycle At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°<br>0% 1 cycle And 70% 25/30 cycles<br>Single phase: at 0<br>0% 300 cycle | 0% 0.5 cycle At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°<br>0% 1 cycle And 70% 25/30 cycles<br>Single phase: at 0<br>0% 300 cycle |
| Power frequency magnetic field<br>IEC 61000-4-8  | 30 A/m<br>50Hz/60Hz  | 30 A/m<br>50Hz/60Hz  |
| Conducted RF<br>IEC 61000-4-6  | 150KHz to 80MHz:<br>3Vrms/6Vrms (in ISM and amateur radio bands)<br>80% Am at 1kHz   | 150KHz to 80MHz:<br>3Vrms<br>6Vrms (in ISM and amateur radio bands)<br>80% Am at 1kHz  |
| Radiated RF<br>IEC 61000-4-3   | 10 V/m<br>80 MHz – 2,7 GHz<br>80 % AM at 1 kHz   | 10 V/m<br>80 MHz – 2,7 GHz<br>80 % AM at 1 kHz   |
| Proximity magnetic fields<br>IEC 61000-4-39  | 30 kHz: 8A/m<br>134.2 kHz: 65A/m<br>13.56 MHz: 7.5A/m  | 30 kHz: 8A/m<br>134.2 kHz: 65A/m<br>13.56 MHz: 7.5A/m  |
| NOTE Ur is the a.c. mains voltage prior to application of the test level.                              |  |  |

Table 3

| Guidance and manufacturer's declaration - electromagnetic Immunity   |                      |             |  |                                     |                   |              |                                |                        |
|--|----------------------|-------------|--|-------------------------------------|-------------------|--------------|--------------------------------|------------------------|
| Radiated RF IEC61000-4-3 (Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment) | Test Frequency (MHz) | Band (MHz)  | Service  | Modulation                          | Maximum Power (W) | Distance (m) | IEC 60601-1-2 Test level (V/m) | Compliance level (V/m) |
|  | 385                  | 380-390     | TETRA 400  | Pulse modulation 18 Hz              | 1,8               | 0,3          | 27                             | 27                     |
|  | 450                  | 430-470     | GMRS 460, FRS 460  | FM $\pm 5$ kHz deviation 1 kHz sine | 2                 | 0,3          | 28                             | 28                     |
|  | 710                  | 704-787     | LTE Band 13,17   | Pulse modulation 217 Hz             | 0,2               | 0,3          | 9                              | 9                      |
|  | 745                  |             |  |                                     |                   |              |                                |                        |
|  | 780                  |             |  |                                     |                   |              |                                |                        |
|  | 810                  | 800-960     | GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5         | Pulse modulation 18 Hz              | 2                 | 0,3          | 28                             | 28                     |
|  | 870                  |             |  |                                     |                   |              |                                |                        |
|  | 930                  |             |  |                                     |                   |              |                                |                        |
|  | 1720                 | 1700 - 1990 | GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3,4, 25; UMTS | Pulse modulation 217 Hz             | 2                 | 0,3          | 28                             | 28                     |
| 1845   |                      |             |  |                                     |                   |              |                                |                        |
| 1970   |                      |             |  |                                     |                   |              |                                |                        |

|  |      |           |  |                               |     |     |    |    |
|--|------|-----------|--|-------------------------------|-----|-----|----|----|
|  | 2450 | 2400–2570 | Bluetooth,<br>WLAN, 802.11<br>b/g/n,<br>RFID 2450,<br>LTE Band 7 | Pulse<br>modulation<br>217 Hz | 2   | 0,3 | 28 | 28 |
|  | 5240 | 5100–5800 | WLAN<br>802.11a/n  | Pulse<br>modulation<br>217 Hz | 0,2 | 0,3 | 9  | 9  |
|  | 5500 |           |  |                               |     |     |    |    |
|  | 5785 |           |  |                               |     |     |    |    |

Table 2

| Guidance and manufacturer's declaration - electromagnetic Immunity  |  |                           |
|---|--|---------------------------|
| Test frequency  | Modulation                               | IMMUNITY TEST LEVEL (A/m) |
| 30 kHz  | CW                                       | 8                         |
| 134,2 kHz   | Pulse modulation <sup>a</sup><br>2,1 kHz | 65 <sup>b</sup>           |
| 13,56 MHz   | Pulse modulation <sup>a</sup><br>50 kHz  | 7,5 <sup>b</sup>          |
| <p>a) The carrier shall be modulated using a 50% duty cycle square wave signal.</p> <p>b) r.m.s., before modulation is applied.</p> |  |                           |

#### **4. Warranty Information**

- The unit is guaranteed to be free of defects in workmanship and materials is used as intended for a period of two years from the date listed on the purchase record.
- For repair under this warranty, our authorized service agent must be advised of the fault within the period of warranty. This warranty covers parts and labor only under normal operations. Any defect resulting from natural cause, e.g Flood, hurricane, etc is not within this guarantee.
- This guarantee does not cover damage incurred by using without following the instructions, accidental damage or being tampered/serviced by unauthorized service agents. A transportation fee or freight fee that may be incurred will be the owner's responsibility.
- This guarantee specifically excludes consumables, for example batteries. All warranty claims must be directed to the distributor responsible for the sale of the device. The content of this warranty is subject to change without further notice.
- Monitor subjected to misuse, abuse and neglect of these manual content excluded from the warranty.
- **WARNING:** No modifications are allowed for this equipment.



U.S. Agent:  
CTI U.S. Inc.  
Suite 230,1455 Cti U.S. Inc.  
Lincoln Parkway, Atlanta, Ga, 30346

Manufacturer:  
 Shenzhen Finicare Co., Ltd  
201, No.50, the 3rd Industrial Park, Houting Community,  
Shajing Street, Bao'an District,  
Shenzhen 518104 China  
E-mail: [info@finicare.com](mailto:info@finicare.com)  
Website: <https://www.finicare.com/>

Made in China